


INSTRUCTION MANUAL

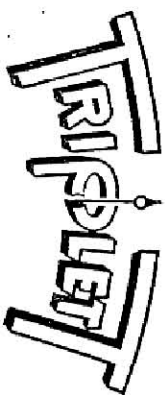


MODEL 850  
ELECTRONIC VOLT-OHM-METER

ABOVE SERIAL 7000

THE TRIPLETT ELECTRICAL INSTRUMENT CO.  
BLUFFTON, OHIO

## TABLE OF CONTENTS

|                                                     |        |
|-----------------------------------------------------|--------|
| TECHNICAL DATA .....                                | Page 4 |
| GENERAL DESCRIPTION .....                           | 5      |
| PRELIMINARY ADJUSTMENTS .....                       | 6      |
| Installing Battery .....                            | 6      |
| Zeroing the Meter .....                             | 6      |
| Warm Up Period .....                                | 6      |
| DC Zero Adjustment .....                            | 6      |
| AC Balance Adjustment .....                         | 7      |
| OPERATING INSTRUCTIONS .....                        | 8      |
| General .....                                       |        |
| AC Voltage Measurements: RMS And Peak To Peak ..... | 8      |
| AF Or Decibel Measurements .....                    | 9      |
| DC Voltage Measurements .....                       | 9      |
| Operation Chart .....                               | 10-11  |
| Resistance Measurements .....                       | 12     |
| Galvanometer Zero Center Scale .....                | 12     |
| MAINTENANCE .....                                   | 13     |
| DC Voltage Calibration .....                        | 13     |
| AC Voltage Calibration .....                        | 15     |
| Ohms Adjustment .....                               | 15     |
| Battery Replacement .....                           | 16     |
| Tube Replacement .....                              | 16     |
| Parts List .....                                    | 17     |
| Schematic Diagram .....                             | 18     |
| WARRANTY .....                                      | 19     |

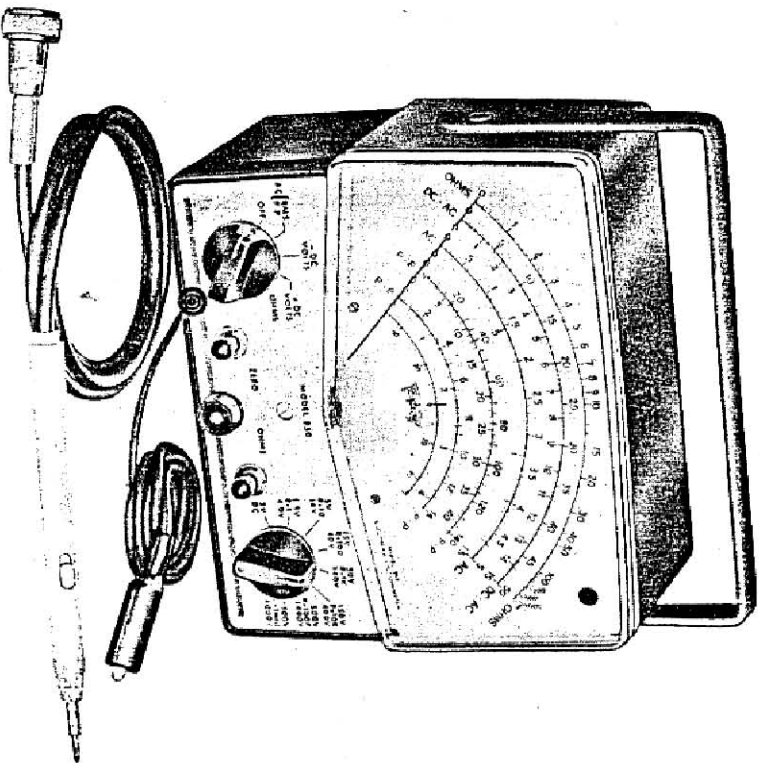

Model 850

**Power**

117 Volts AC 50-60 cps; power consumption 6 Watts.

**Ranges**

DC Volts 0-.5-1.5-5-15-50-150-500-1500  
 AC Volts 0-1.5-5-15-50-150-500-1500  
 Peak to Peak 0-4-14-40-140-400-1400-4,000  
 Ohms 0-1000-10,000-100,000-1 Meg.-10 Meg.-100 Meg.-1000 Meg.

**Frequency Range**

15 CPS to 3 MC; up to 250 MC with accessory diode probe.

**Input Impedance**

DC Volts 11 Megohms—AC Volts minimum of .83 Megohm.

**Meter**

DC current for full scale deflection 200  $\mu$ a meter.  
 7 inch type with 7 inch scale length.  
 DC - AC RMS scale black on white.  
 Ohms scale black on white.  
 Peak to Peak scale red on white.

**Accuracy**

AC  $\pm 3\%$ , DC  $\pm 3\%$

**Tube Complement**

1 — 12AU7, 1 — 6AL5.

**Construction**

Insulated black case; dimension outside  $7\frac{3}{4}'' \times 6\frac{7}{16}'' \times 3\frac{3}{4}''$   
 with metal handle that can be used to place instrument on  
 a  $25^\circ$  angle. Etched aluminum panel.

**Weight**

Approximately 5 pounds.

**Accessories supplied with Model 850**

1 DC/AC - CHMS probe and cable  
 1 Chassis ground lead  
 1 1.5 Volt battery  
 1 Alligator clip  
 1 Instruction book

**Accessories Available**

DC High Voltage probe 79B-196  
 RF probe 79A-215  
 Leather Carrying Case

**GENERAL DESCRIPTION**

The Electronic Volt-Ohmmeter is one of the most useful instruments in the electronic field, both in the laboratory and for service. Its high input impedance and wide frequency ranges give it considerable advantage over other types of voltmeters. The versatility of a Triplett Model 850 is greatly increased by the skill of the operator.

The 850 is an electronic voltmeter designed to measure DC voltages, resistance, AC RMS and peak to peak value. By adding color to the various ranges the meter dial is easy to read. Your 850 is designed with added protection for the highly sensitive meter. By special circuit arrangement the meter is shorted out in the OFF position for greater damping and meter safety during transit. The black molded case is completely insulated and has a plastic covered handle that can be used to place the instrument on a  $25^\circ$  angle.

The meter controls are clearly marked on an etched aluminum panel. All measurements are made on a seven-inch meter with separate red scales for peak to peak voltages.

One probe is used for all functions: DC, AC and OHMS. The small compact probe has a built-in sliding switch which places a one megohm resistor in series with the instrument on DC voltage readings. The 850 is frequency compensated up to 3 megacycles. Up to 250 MC can be measured with an RF probe obtainable on special order.

You will find four, black rubber feet inside of the envelope holding the probe. These feet are part of the tester, and are to be placed in the four holes at the rear of the case.

## PRELIMINARY ADJUSTMENTS

The following procedure and adjustments should be made before using your Model 850. In following this procedure, you will familiarize yourself with the 850 and at the same time, increase the efficiency of the 850 and your use of it.

### Installing Battery

1. Remove the five screws in the rear of the case, and pull the tester out of the case.
2. Install the battery (Eveready #935 or Burgess #1) observing the + polarity marking on the battery holder.

### Zeroing the Meter

This is the mechanical adjustment of the meter, and is to be done with no power applied to the tester.

1. Place tester in vertical position.
2. Adjust the meter adjustment screw for exact zero meter indication.

### Warm Up Period

1. Plug tester line cord into 117 a-c volt outlet and turn function switch to +D.C. Volts position.
2. Allow to warm up for 15 minutes.

### D. C. Zero Adjustment

1. Connect probe cable to front panel connector, and place slide switch in DC position; connect the probe tip and long black ground lead together, which grounds the input of the VTVM.

2. Index the range switch to 1.5 volt position.
3. Adjust the front panel zero control (control to the left of the connector) until the meter is indicating exactly zero.
4. Turn the function switch to -D.C. Volts position. The meter reading should remain at exactly zero. If this is not true, repeat step Zeroing of the Meter above.

### A. C. Balance Adjustment

1. If case is connected to panel, again remove the five screws from the back of the case and slide the panel approximately an inch out of the case. Note the row of calibration controls on top of the chassis, and that each control is plainly marked.
2. Tester must be on exact D. C. zero as mentioned in paragraph on Zero Adjustment.
3. Turn Function switch to A. C. Volts position. NOTE: Do NOT readjust the front panel zero control.
4. Place slide switch on probe to AC position, and probe is still to be shorted to the ground lead.
5. Note the A. C. Zero control, which is at one end of the row of controls inside the tester. This is the control closest to the neon lamp. Adjust this control until the pointer indicates exactly zero on the meter.
6. After this adjustment, changing from A. C. to D. C. volt indexes should not change the zero indication of the meter.

OPERATING INSTRUCTIONS

General

1. Connect DC/AC OHMS probe and cable to the front panel connector.
2. Plug the line cord into a 117 volt 60 cycle power outlet.
3. Check and adjust mechanical zero if necessary.
4. Turn function selector to DC VOLTS and allow at least 2 minutes to warm up.
5. Adjust electrical ZERO control to position on left hand zero on meter. Probe tip should be shorted to ground when adjusting electrical zero.
6. Turn function selector to OHMS position and adjust to full scale with OHMS control.
7. Red scale is for peak to peak readings—Black AC—DC—OHMS.
8. CAUTION: Do not use the common ground (black ground lead) in excess of 400 Volts AC, or 600 Volts DC from earth ground.
9. Tester is now ready for use.


AC Voltage Measurements: RMS and Peak to Peak

The probe switch should be in the AC-OHMS position for all AC voltage measurements. Peak to Peak voltage values are read from the red scales; RMS values are read from the black scales.

1. Set the function selector to AC.
2. Adjust the zero control to position the meter pointer at the left hand "0".
3. Select a higher voltage range than the voltage to be measured.
4. Connect the ground clip to ground (or the lowest potential of circuit under test.)
5. Connect the probe tip to the other side of the voltage.
6. Reset the range switch for a reading nearest full scale.

AF or Decibel Measurements

To measure decibels set the tester as above for AC Volts RMS. Convert the RMS readings to decibels with the chart below.

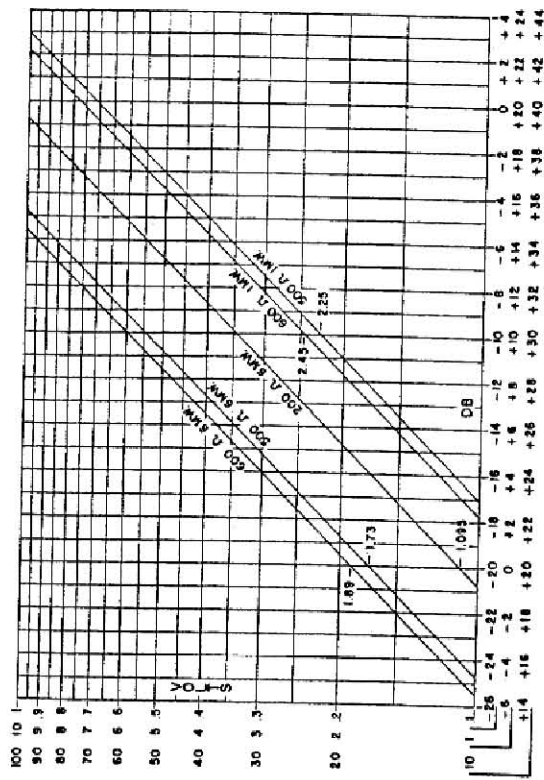

DC Voltage Measurements

On all DC voltage measurements the switch on the DC/AC OHMS probe should be in the DC position.

The probe is positive when the selector switch is in the +DC Volts position and negative when in the -DC Volts position.

1. Select the correct function; +DC Volts or -DC Volts.
2. Select a higher voltage range than the voltage to be measured.

(Continued on page 12)

| TO MEASURE           | SET RANGE SWITCH AT | SET FUNCTION SWITCH AT | PROBE SWITCH POSITION | READ ON SCALE   | SCALE       | REMARKS                                                                             |                                                                                        |
|----------------------|---------------------|------------------------|-----------------------|-----------------|-------------|-------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------|
| DC Volts             |                     |                        |                       | Black Scales    |             |                                                                                     |                                                                                        |
| 0-.5                 | .5                  | DC VOLTS               | DC                    | 0-50 DC         | ÷ by 100    | See instructions for DC Volts measurements. Be sure probe switch is in DC position. |                                                                                        |
| 0-1.5                | 1.5                 | DC VOLTS               | DC                    | 0-15 DC         | ÷ by 10     |                                                                                     |                                                                                        |
| 0-5                  | 5                   | DC VOLTS               | DC                    | 0-50 DC         | ÷ by 10     |                                                                                     |                                                                                        |
| 0-15                 | 15                  | DC VOLTS               | DC                    | 0-15 DC         | Read Direct |                                                                                     |                                                                                        |
| 0-50                 | 50                  | DC VOLTS               | DC                    | 0-50 DC         | Read Direct |                                                                                     |                                                                                        |
| 0-150                | 150                 | DC VOLTS               | DC                    | 0-15 DC         | x 10        |                                                                                     |                                                                                        |
| 0-500                | 500                 | DC VOLTS               | DC                    | 0-50 DC         | x 10        | See instructions for AC RMS measurements.                                           |                                                                                        |
| 0-1500               | 1500                | DC VOLTS               | DC                    | 0-15 DC         | x 100       |                                                                                     |                                                                                        |
| AC-RMS               |                     |                        |                       | Black Scales    |             |                                                                                     |                                                                                        |
| 0-1.5                | 1.5                 | AC-RMS                 | AC-OHMS               | 0-1.5 AC        | Direct      |                                                                                     | See instructions for resistance measurements. Be sure probe switch is in OHM position. |
| 0-5                  | 5                   | AC-RMS                 | AC-OHMS               | 0-5 AC          | Direct      |                                                                                     |                                                                                        |
| 0-15                 | 15                  | AC-RMS                 | AC-OHMS               | 0-15 AC         | Direct      |                                                                                     |                                                                                        |
| 0-50                 | 50                  | AC-RMS                 | AC-OHMS               | 0-50 AC         | Direct      |                                                                                     |                                                                                        |
| 0-150                | 150                 | AC-RMS                 | AC-OHMS               | 0-15 AC         | x 10        |                                                                                     |                                                                                        |
| 0-500                | 500                 | AC-RMS                 | AC-OHMS               | 0-50 AC         | x 10        |                                                                                     |                                                                                        |
| 0-1500               | 1500                | AC-RMS                 | AC-OHMS               | 0-15 AC         | x 100       | See instructions for Peak to Peak voltage measurement.                              |                                                                                        |
| OHMS                 |                     |                        |                       | Top Scale OHMS  |             |                                                                                     |                                                                                        |
| 0-1000               | R x 1               | OHMS                   | AC-OHMS               | 0-1000 OHMS     | Read Direct |                                                                                     | See instructions for Decibel measurements.                                             |
| 0-10,000             | R x 10              | OHMS                   | AC-OHMS               | 0-1000 OHMS     | x 10        |                                                                                     |                                                                                        |
| 0-100,000            | R x 100             | OHMS                   | AC-OHMS               | 0-1000 OHMS     | x 100       |                                                                                     |                                                                                        |
| 0-1,000,000          | R x 1K              | OHMS                   | AC-OHMS               | 0-1000 OHMS     | x 1K        |                                                                                     |                                                                                        |
| 0-10,000,000         | R x 10K             | OHMS                   | AC-OHMS               | 0-1000 OHMS     | x 10K       |                                                                                     |                                                                                        |
| 0-100 Meg.           | R x 100K            | OHMS                   | AC-OHMS               | 0-1000 OHMS     | x 100K      |                                                                                     |                                                                                        |
| 0-1000 Meg.          | R x 1 Meg.          | OHMS                   | AC-OHMS               | 0-1000 OHMS     | x 1 Meg.    | See instructions for Decibel measurements.                                          |                                                                                        |
| Peak to Peak         |                     |                        |                       | Red Scales      |             |                                                                                     |                                                                                        |
| 0-4 *                | 4                   | AC-PP                  | AC-OHMS               | 0-4 PP          | Read Direct |                                                                                     | See instructions for Decibel measurements.                                             |
| 0-14                 | 14                  | AC-PP                  | AC-OHMS               | 0-14 PP         | Read Direct |                                                                                     |                                                                                        |
| 0-40                 | 40                  | AC-PP                  | AC-OHMS               | 0-40 PP         | Read Direct |                                                                                     |                                                                                        |
| 0-140                | 140                 | AC-PP                  | AC-OHMS               | 0-140 PP        | Read Direct |                                                                                     |                                                                                        |
| 0-400                | 400                 | AC-PP                  | AC-OHMS               | 0-40 PP         | x 10        |                                                                                     |                                                                                        |
| 0-1400               | 1400                | AC-PP                  | AC-OHMS               | 0-140 PP        | x 10        |                                                                                     |                                                                                        |
| 0-4000               | 4000                | AC-PP                  | AC-OHMS               | 0-40 PP         | x 100       | See instructions for Decibel measurements.                                          |                                                                                        |
| Decibels             |                     |                        |                       | Black AC Scales |             |                                                                                     |                                                                                        |
| See Chart -26 to +40 | 1.5                 | AC-RMS                 | AC-OHMS               | Black AC Scales |             |                                                                                     |                                                                                        |
|                      | 5                   | AC-RMS                 | AC-OHMS               |                 |             |                                                                                     |                                                                                        |
|                      | 15                  | AC-RMS                 | AC-OHMS               |                 |             |                                                                                     |                                                                                        |
|                      | 50                  | AC-RMS                 | AC-OHMS               |                 |             |                                                                                     |                                                                                        |
|                      | 150                 | AC-RMS                 | AC-OHMS               |                 |             |                                                                                     |                                                                                        |

3. Connect the ground clip to ground (or the lowest potential of circuit under test.)
4. Connect the probe tip to the high side of the voltage to be measured.
5. Set the range switch to the position that gives a reading nearest full scale.
6. The DC voltage is then read on the scale corresponding to the range setting.

#### Resistance Measurements

The probe switch should be in the AC OHMS position when resistance measurements are made. Power must be removed from equipment under test before resistance measurements are made.

1. Set function switch to the OHMS position.
2. Set range switch to the Rx10 position.
3. Short the probe tip to the ground cable and adjust the ZERO control to position the pointer at the left-hand "0".
4. Separate the probe tip from the ground cable. Adjust the meter pointer to full scale with the OHMS control.
5. Connect the ground cable clip to one side of the resistance to be measured.
6. Connect the probe tip to the other side of the resistance to be measured.
7. Reset the range control to give a convenient deflection on the OHMS scale.
8. After resetting the range control repeat steps three and four.
9. Multiply the reading on the OHMS scale by the range switch setting.

#### Galvanometer Zero Center Scale

Zero center scale is available for lining up the discriminator in FM circuits or for other Galvanometer readings.

To use the Zero Center Scale as a Galvanometer:

1. Set the function switch to "+DC Volts".
2. Adjust the ZERO control to position the pointer at the "-0+" which is at the bottom of the meter scale.
3. Set the range selector to a position at least twice the voltage to be measured.
4. Full scale readings will be half the value of the range setting since "0" is in center of the meter.

Example: If range switch is on 5 DCV and "0" is in center of meter, the meter will read -2.5, 0, +2.5 Volts.

#### MAINTENANCE

##### DC Voltage Calibration

1. Zero the mechanical meter zero.
2. Set on +DC Volts position and allow 15 minutes minimum warm up.
3. Line voltage should be 117 Volts 60 CPS.
4. Zero the electrical zero.
5. Set on 50 Volt position.
6. Set the probe switch on DC position.
7. Connect ground lead of 850 to negative side of 50 Volt DC standard source. Connect positive side of source to probe tip.
8. Adjust the +DC cal. potentiometer so the meter reads exactly 50 Volts full scale.
9. Reverse the test lead connections at the voltage sources.
10. Set switch to -DC Volts.
11. Adjust the -DC cal. potentiometer so the meter reads exactly 50 Volts full scale.
12. Check the remaining DC voltage ranges with a standard voltage source.

13. Index Range switch to .5 DC position, and turn Function switch to  $\pm$  DC Volts.
14. Connect probe lead and ground leads together and zero tester.
15. Connect leads across a standard .5 DC voltage supply, and adjust pointer to a full scale reading by means of the control marked  $\pm .5$  and located in the row of controls on the chassis.
16. Disconnect leads, turn Function switch to  $-$  DC volts, and connect leads to standard .5 DC voltage supply, connecting the leads in just the opposite manner than in step 15 above.
17. Adjust the  $- .5$  control on the chassis until the pointer is on the full scale mark on the meter.

### AC Voltage Calibration


1. Set the probe switch to the AC/OHMS position.
2. Set on AC Volt position.
3. Set on 1.5 Volt range.
4. Short the probe tip to ground and adjust the AC Zero potentiometer so the meter reads exactly zero. If zero cannot be obtained, replace the 6AL5 tube. (Use only RCA or Sylvania).
5. Set on the 50 Volt range.
6. Apply 50 Volts 60 CPS to the probe tip and ground lead.
7. Adjust the AC cal. control so the meter reads exactly 50 Volts full scale.
8. Check the remaining AC voltage ranges with a standard voltage source.

### Ohms Adjustment

1. Set the 850 to the  $\pm$ DC Volts position and zero if necessary.
2. Set to OHMS position.
3. Set to Rx1 range.
4. Adjust OHMS control for full scale.

NOTE: In areas where the line voltage is not 117 Volts, it may be desirable to readjust the AC Zero potentiometer so that the DC and AC ranges automatically balance at the same point. To do this:

1. Set on DC $\pm$  position and allow 15 minutes to warm up.
2. Set probe to DC, short probe to ground, and adjust to zero with electrical zero control.
3. Set probe to AC/OHMS position.
4. Set selector on AC Volt position.
5. Short probe to ground. Do not move electrical zero. Adjust to zero by means of the AC Zero potentiometer, which is the control nearest the neon light, on the inside of the tester.



## Battery Replacement

The 1.5 Volt battery is used for resistance measurements only. If unable to adjust pointer to full scale on the R x 1 range, the battery should be replaced with Eveready #935, Burgess #1 or equivalent.

## Tube Replacement

Should it become necessary to replace a tube, the following procedure should be followed. The tubes in the Model 850 have been aged and selected before being put into use. Select a 12AU7 tube that after a 15 minute warm up period is fairly stable when switching from one DC range to another. After tube selection it should be aged in the 850 for 100 hours. Sometimes it is possible that a tube will prove unstable after being aged. In such case the procedure must be repeated.

When replacing the 6AL5 it is only necessary to age it 100 hours in the 850 with the power turned on. This should be replaced by only RCA or Sylvania 6AL5 tubes.

When replacing either or both tubes it is necessary for the calibration to be checked as outlined in the DC voltage calibration and AC voltage calibration procedure under maintenance.

We recommend that all major recalibrating and repairs be done by the manufacturer. Our meter maintenance department is at your service. When necessary to return your instrument for repair, please write for return authorization.

## REPLACEABLE PARTS 850

| REC.        | DESCRIPTION                                                       | TRIPLETT<br>PART NO. |
|-------------|-------------------------------------------------------------------|----------------------|
| B1          | Load Assem. 850 Chassis Ground                                    | 79A-214              |
| P1          | Load Assem. 850 Probe                                             | 79B-192              |
| T1          | Battery 1.5 volts Eveready 935 or equal                           | T-2426-2             |
| L1          | Power Cord                                                        | T-2566A-51           |
| X1          | Transformer                                                       | 22A-175              |
| V1          | Neon Lamp, NE-2H                                                  | 67-98                |
| V2          | Rectifier, ERLE ED3003                                            | T-2250-55            |
| C2          | Capacitor, Dry Electrolytic 12 mfd., 250V                         | T-3238-1             |
| C3          | Capacitor, Tubular 1 mfd. $\pm 20\%$ , 100V                       | T-2500-5AL5          |
| C5 & C7     | Capacitor, Tubular .05 mfd. $\pm 20\%$ , 400V                     | T-2600-12AU7         |
| C1, C4 & C8 | Capacitor, Ceramic Disc, 0.01 mfd., 600 WVDC                      | 34-48                |
| S1          | Switch, Function                                                  | 43-242               |
| S2          | Switch Assembly with Resistor Function                            | 43-235               |
| S3          | Switch Selector                                                   | T-43-37              |
| R1          | Resistor, 10K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | 43-198               |
| R2          | Resistor, 20K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | 22A-391              |
| R3          | Resistor, 30K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | 22A-361              |
| R4          | Resistor, 40K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | 22A-390              |
| R5          | Resistor, 50K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | 22-362               |
| R6          | Resistor, 60K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | T-15-2921            |
| R7          | Resistor, 70K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | T-15-3232            |
| R8          | Resistor, 80K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | 15-3802              |
| R9          | Resistor, 90K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type       | 15-3807              |
| R10         | Resistor, 100K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3901              |
| R11         | Resistor, 110K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3903              |
| R12         | Resistor, 120K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | T-15-3390            |
| R13 & R14   | Resistor, 130K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3296              |
| R15         | Resistor, 150K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | T-15-2474            |
| R16         | Resistor, 160K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 16-131               |
| R17         | Resistor, 170K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 16-141               |
| R18         | Resistor, 180K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-2507              |
| R19         | Resistor, 190K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 37-11                |
| R20         | Resistor, 200K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | T-15-1873            |
| R21 & R22   | Resistor, 220K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 16-133               |
| R23         | Resistor, 240K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-1456              |
| R24         | Resistor, 250K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-1115              |
| R25         | Resistor, 270K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 16-147               |
| R26         | Resistor, 300K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-1411              |
| R27         | Resistor, 330K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-2925              |
| R28         | Resistor, 360K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3004              |
| R29         | Resistor, 390K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3005              |
| R30         | Resistor, 420K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3298              |
| R31         | Resistor, 450K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-324               |
| R32         | Resistor, 480K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 6524                 |
| R33         | Resistor, 510K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-1482              |
| R34         | Resistor, 560K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | T-2501-12-100        |
| R35         | Resistor, 620K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3639              |
| R36         | Resistor, 680K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-2930              |
| R37         | Resistor, 750K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3286              |
| R38         | Resistor, 820K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3289              |
| R39         | Resistor, 910K ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3391              |
| R40         | Resistor, 1M ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type        | 15-3301              |
| R41         | Resistor, 1.1M ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3307              |
|             | Resistor, 1.2M ohm $\pm 1\%$ , $\frac{1}{2}$ watt, Film Type      | 15-3297              |
|             | Resistor, 1.5 meg ohm $\pm 5\%$ , $\frac{1}{2}$ watt, Composition | 10A-1296             |
|             | Case Assem.                                                       | 10A-1295             |
|             | Front Assem.                                                      | 10A-1295             |

# TRIPLETT WARRANTY AND CONDITIONS OF SALE


The Triplett Electrical Instrument Company warrants instruments manufactured by it to be free from defective material or factory workmanship and agrees to repair or replace such instruments which under normal use and service, disclose the defect to be the fault of our manufacturing. Our obligation under this warranty is limited to repairing or replacing any instrument or test equipment which proves to be defective, when returned to us transportation prepaid, within ninety (90) days from the date of original purchase.

This warranty does not apply to any of our products which have been repaired or altered by unauthorized persons or service stations in any way so as, in our judgment, to injure their stability or reliability or which have been subject to misuse, negligence, or accident, or which have had the serial number altered, effaced, or removed. Neither does this warranty apply to any of our products which have been connected, installed, or adjusted otherwise than in accordance with the instructions furnished by us. Accessories including all vacuum tubes and batteries not of our manufacture used with this product are not covered by this warranty.

The Triplett Electrical Instrument Company reserves the right to discontinue models at any time, or change specifications or design, without notice and without incurring any obligation.

Upon acceptance of the material covered by this invoice the purchaser agrees to assume all liability for any damages and bodily injury which may result from the use or misuse of the material by the purchaser, his employees, or others, and that The Triplett Electrical Instrument Company shall incur no liability for direct or consequential damage of any kind.

Parts will be made available for a maximum period of five (5) years after the manufacture of this equipment has been discontinued. Parts include all materials, charts, instructions,

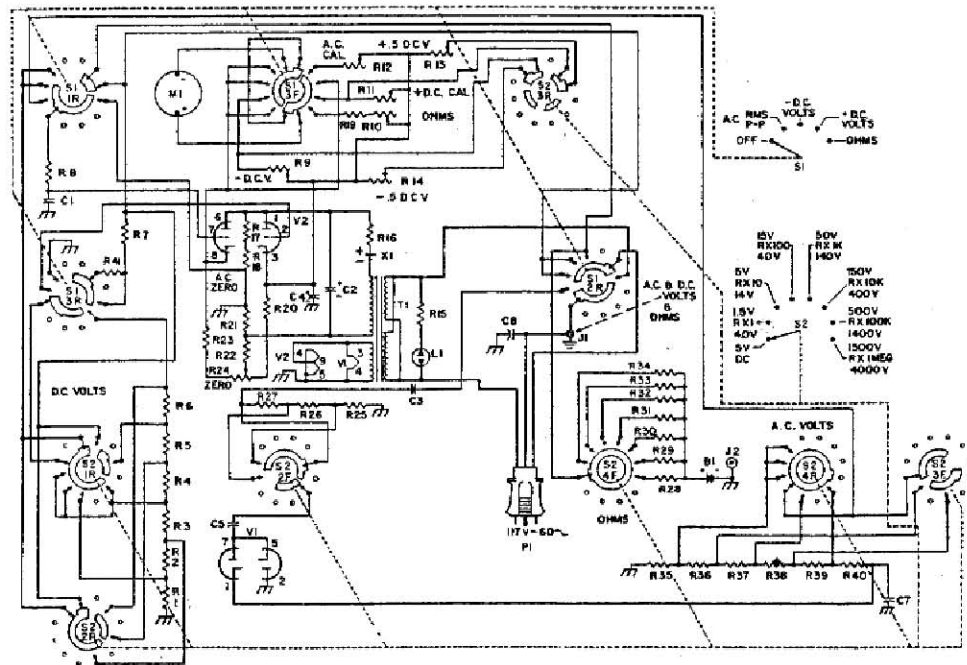

diagrams, accessories, et cetera, which were furnished in the standard or special models.

This warranty and conditions of sale are in lieu of all others expressed or implied and no representative or person is authorized to assume for us any other liability in connection with the sale of our products.

THE TRIPLETT ELECTRICAL INSTRUMENT COMPANY

Bluffton, Ohio

Printed in U. S. A.

Part No. 84-112-102364-14